

POLARIMETER: A Soft X-Ray 8-Axis UHV-Diffractometer at BESSY II

Helmholtz-Zentrum Berlin für Materialien und Energie *

Instrument Scientists:

- Dr. Andrey Sokolov, Helmholtz-Zentrum Berlin für Materialien und Energie, phone: +49 30 8062-12986, email: andrey.sokolov@helmholtz-berlin.de
- Dr. Franz Schäfers, Helmholtz-Zentrum Berlin für Materialien und Energie, phone: +49 30 8062-12946, email: franz.schaefers@helmholtz-berlin.de

Abstract: A versatile UHV-polarimeter for the EUV XUV spectral range is described which incorporates two optical elements: a phase retarder and a reflection analyzer. Both optics are azimuthally rotatable around the incident synchrotron radiation beam and the incidence angle is freely selectable. This allows for a variety of reflectometry, polarimetry and ellipsometry applications on magnetic or non-magnetic samples and multilayer optical elements.

1 Introduction

The high precision 8-axis ultra-high vacuum compatible (UHV)-polarimeter (Schäfers et al., 1999) is a multipurpose instrument which can be used as a multilayer-based self-calibrating polarization detector for linearly and circularly polarized UV- and soft X-ray light (Gaupp et al., 2013; MacDonald et al., 2009). It can also be used for the characterization of either reflection or transmission properties (reflectometry) (Eriksson et al., 2006; Schäfers, 2000) as well as to determine polarizing and phase retarding properties (ellipsometry) of any optical element (Uschakow et al., 2013). Magneto-optical experiments are possible in transmission, as the XMCD or XMLD (Magnetic Circular / Linear Dichroism) that are intensity measurements (Mertins et al., 2002).

Additionally a polarization analysis of the transmitted or reflected light is possible which allows for Faraday-, Voigt- or Kerr-effect technique (L-MOKE, T-MOKE) to investigate thin films as well as magnetic multilayers (Mertins et al., 2001; Zaharko et al., 2002). Independent two-dimensional rotation of the detector enables any non-specular magnetic scattering experiment on magnetic dots or grains. A load-lock transfer chamber allows for quick and easy sample exchange.

*Cite article as: Helmholtz-Zentrum Berlin für Materialien und Energie. (2016). POLARIMETER: A Soft X-Ray 8-Axis UHV-Diffractometer at BESSY II. *Journal of large-scale research facilities*, 2, A92. <http://dx.doi.org/10.17815/jlsrf-2-90>

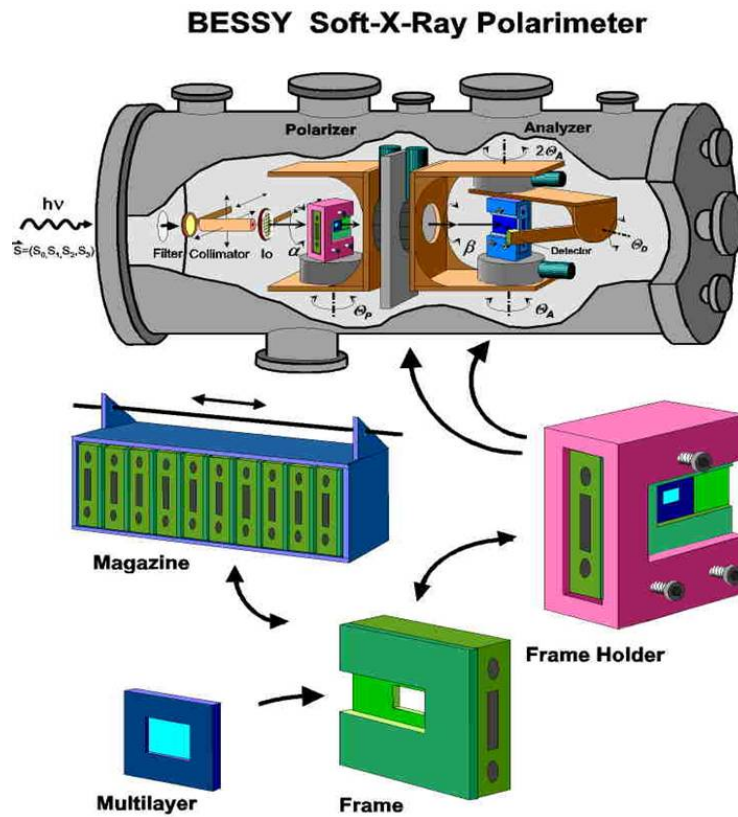


Figure 1: Schematic view of the POLARIMETER station.

2 Instrument application

Typical applications are:

- Characterization of optical elements
- Reflection, transmission properties (s-, p-pol.)
- Polarizing properties (phase retardation)
- Determination of polarization of incident light (Stokes $S_0, 1, 2, 3$)
- Resonant Magnetic Scattering (specular and diffuse)
- Intensity spectroscopy: MCD, LMD, Kerr-effect (L, T-MOKE)
- Polarization spectroscopy: Faraday-, Voigt, Kerr-effect

Methods:

- Elipsometry
- Polarimetry
- Reflectometry

3 Technical Data

Experiment in vacuum	10^{-9} mbar
Temperature range	280 - 480 K
Max. sample size	$50 \times 50 \times 11 \text{ mm}^3$
Min. sample size	$10 \times 10 \times 0.5 \text{ mm}^3$
Incidence angle scan range	$0^\circ \leq \Theta_P, \Theta_A \leq 90^\circ$
Azimuthal angle scan range	$0^\circ \leq \alpha, \beta \leq 370^\circ$
Detector scan range (in plane)	$0^\circ \leq \Theta_{2A} \leq 180^\circ$
(off-plane)	$-10^\circ \leq \Theta_D \leq 27^\circ$
Min. step size for all motors	0.001°
Sample – Detector Distance	150 mm
Magnetic fields (in-/off-plane) (long./transv.)	$-450 < H < 450$ Oe
Detector	GaAsP-photodiode with Keithley electrometer 617 (6514)
Detector size	$4 \times 4 \text{ mm}^2, 0.2 \times 4 \text{ mm}^2$
Load-lock, Magazine	<i>In-situ</i> storage of up to 10 samples
Higher order filters	Be, B, C ₆ H ₈ , Ti, Cr, Fe
Collimator pinholes	$\varnothing 0.2 - 2.0$ mm

Table 1: Technical data of the POLARIMETER station.

References

- Eriksson, F., Ghafoor, N., Schäfers, F., Gullikson, E. M., & Birch, J. (2006). Interface engineering of short-period Ni/V multilayer X-ray mirrors. *Thin Solid Films*, 500(1-2), 84 - 95. <http://dx.doi.org/10.1016/j.tsf.2005.11.019>
- Gaupp, A., Schäfers, F., MacDonald, M., Uschakow, S., Salashchenko, N. N., & Gaykovich, P. K. (2013). Carbon K-edge polarimetry with Cr/Sc multilayers. *Journal of Physics: Conference Series*, 425(12), 122013. <http://dx.doi.org/10.1088/1742-6596/425/12/122013>
- MacDonald, M. A., Schäfers, F., & Gaupp, A. (2009). A single W/B4C transmission multilayer for polarization analysis of soft x-rays up to 1keV. *Opt. Express*, 17(25), 23290–23298. <http://dx.doi.org/10.1364/OE.17.023290>
- Mertins, H.-C., Abramsohn, D., Gaupp, A., Schäfers, F., Gudat, W., Zaharko, O., ... Oppeneer, P. M. (2002). Resonant magnetic reflection coefficients at the Fe 2p edge obtained with linearly and circularly polarized soft x rays. *Phys. Rev. B*, 66, 184404. <http://dx.doi.org/10.1103/PhysRevB.66.184404>
- Mertins, H.-C., Oppeneer, P. M., Kuneš, J., Gaupp, A., Abramsohn, D., & Schäfers, F. (2001). Observation of the X-Ray Magneto-Optical Voigt Effect. *Phys. Rev. Lett.*, 87, 047401. <http://dx.doi.org/10.1103/PhysRevLett.87.047401>
- Schäfers, F., Mertins, H.-C., Gaupp, A., Gudat, W., Mertin, M., Packe, I., ... Eriksson, M. (1999). Soft-x-ray polarimeter with multilayer optics: complete analysis of the polarization state of light. *Appl. Opt.*, 38(19), 4074–4088. <http://dx.doi.org/10.1364/AO.38.004074>
- Schäfers, F. (2000). Multilayers for the EUV/soft X-ray range. *Physica B: Condensed Matter*, 283(1-3), 119 - 124. [http://dx.doi.org/10.1016/S0921-4526\(99\)01903-1](http://dx.doi.org/10.1016/S0921-4526(99)01903-1)



Uschakow, S., Gaupp, A., MacDonald, M., & Schäfers, F. (2013). EUV Ellipsometry on Mo/Si Multilayers. *Journal of Physics: Conference Series*, 425(15), 152011. <http://dx.doi.org/10.1088/1742-6596/425/15/152011>

Zaharko, O., Oppeneer, P. M., Grimmer, H., Horisberger, M., Mertins, H.-C., Abramsohn, D., ... Braun, H.-B. (2002). Exchange coupling in fe/nio/co film studied by soft x-ray resonant magnetic reflectivity. *Phys. Rev. B*, 66, 134406. <http://dx.doi.org/10.1103/PhysRevB.66.134406>